


FK-26888-000

THE FK-26888-000 IS AN UNDAMPED MAGNETIC BALANCED ARMATURE RECEIVER INTENDED FOR USE IN CIC HEARING INSTRUMENTS. THIS MODEL HAS HIGH PERMEABILITY CUP & COVER TO REDUCE MAGNETIC RADIATION, AND HAS THE CENTER TERMINAL ELECTRICALLY CONNECTED TO CASE.

CONSTANT VOLTAGE DRIVE CONDITIONS

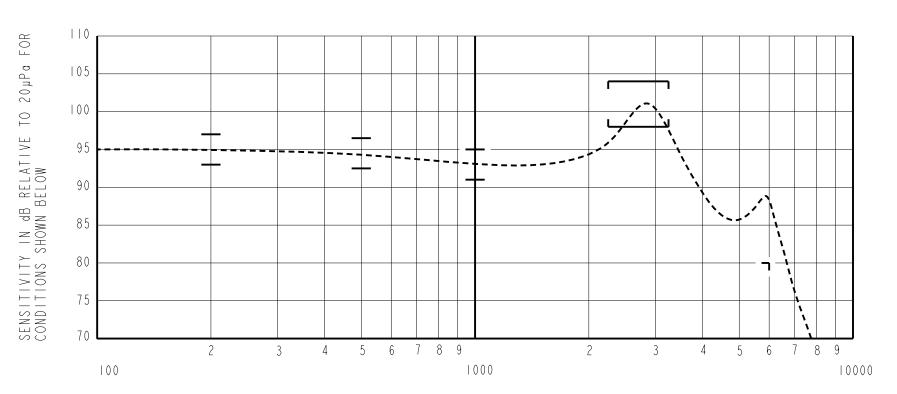

FREQUENCY IN HERTZ

ACOUSTICAL

SENSITIVITY

DEVICE WILL PRODUCE THE SPL LISTED BELOW UNDER TEST CONDITIONS DESCRIBED IN TABLE 3. NOMINAL SENSITIVITY AT IKHZ IS dB RELATIVE TO 20µPa. ALL OTHER VALUES IN dB RELATIVE TO THE SENSITIVITY AT IKHZ.

FREQUENCY (Hz)	MINIMUM	NOMINAL	MAXIMUM
200	0.0	+2.0	+4.0
500	-0.5	+1.5	+3.5
1000	-2.0	93.0	+2.0
2250 - 3250	+5.0	+8.0	+ .0
6000	80.0		

TABLE I

TOTAL HARMONIC DISTORTION

DEVICE WILL NOT EXCEED TOTAL HARMONIC DISTORTION LEVELS LISTED BELOW.

FREQUENCY (Hz)	AC DRIVE (V rms)	DC BIAS (mA)	LIMIT (%)
920	0.367	0	5
1380	0.367	0	5
920	1.04	0	10

TABLE 2

TEST CONDITIONS

TEST CONDITIONS		
NOMINAL SOURCE VOLTAGE	0.367 V rms, 0 mA DC BIAS	
SOURCE IMPEDANCE	Ohm</td	
TUBING		
COUPLER CAVITY	2 CM ³ , SIMULATED ANSI S3.7 TYPE HA-3 (IEC 60318-5)	

TABLE 3

ELECTRICAL

DC RESISTANCE	580 Ohms ± 10%
IMPEDANCE @ 500 Hz	690 Ohms ± 15%
IMPEDANCE @ IkHz	940 Ohms ± 15%

TABLE 4

ISOLATION: CASE WILL BE ELECTRICALLY ISOLATED FROM THE COIL CIRCUIT.

	Revision	C.O. #	Implementation Date	RELEASE LEVEL		REVISION
						_
	E	C10114032	11-7-12	Active		F 1
	D	C10112265	3-31-11			
		WHEN TEST LIMITS ARE USED TO ESTABLISH INCOMING INSPECTION ACCEPTANCE/REJECTION			DR. BY	DATE
7.00	CRITERIA, CORRELATION OF TEST EQUIPMENT WITH KNOWLES IS ALSO REQUIRED FOR ELIMINATION OF EQUIPMENT AND TEST METHOD VARIATION				МММ	7 - 3 I - 06
ICS					CK. BY	DATE
	TITLE:	RF	CEIVER	FK-26888-000	GJP	8 - 4 - 06
	1 10011111			APP. B		DATE
		PERFORMAN	NCE SPECIFICATION	SHT 2.1	GJP	8 - 4 - 06

PORT LOCATION: 3S

TEMPERATURE

SOLDER TYPE: SAC305

OPERATURE: SENSITIVITY WILL NOT VARY

-17°C TO 63°C.

STORAGE: -40°C TO 63°C.

MORE THAN +1/-3 dB FROM

KNOWLES ELECTRONICS
ITASCA, ILLINOIS U.S.A.